




Pituitary Rongeur with Teeth

Designed by Michael Murray, MD

Designed to optimize the efficiency of soft tissue removal and disc space preparation prior to a spinal interbody fusion

Unique design ensures that only the distal tip of the instrument is in contact upon closure of the jaws, allowing the grasping force to be optimized, and directed at the distal tip of the instrument. In addition, the teeth at the distal end of the instrument allow for a better grasp on tissues or disc material, for enhanced control and efficiency of removal.

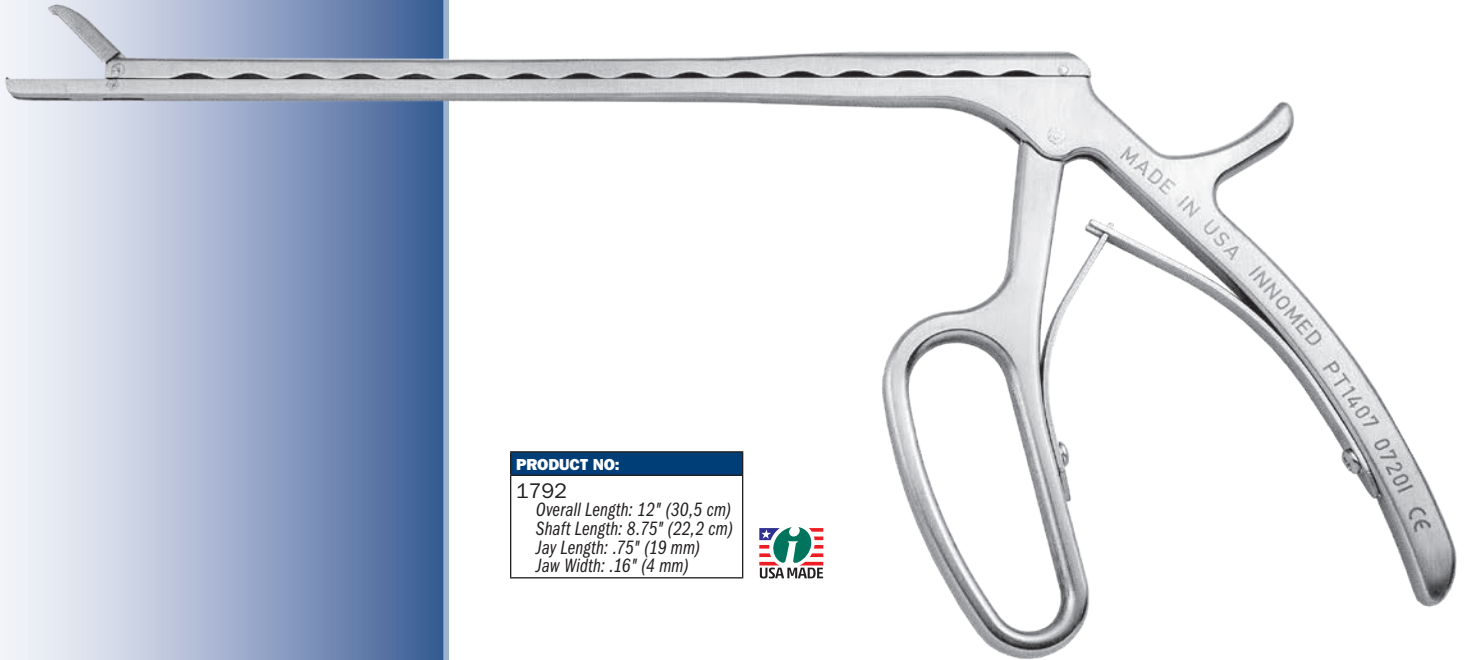

PRODUCT NO:

1792
Overall Length: 12" (30,5 cm)
Shaft Length: 8.75" (22,2 cm)
Jaw Length: .75" (19 mm)
Jaw Width: .16" (4 mm)



ISO 13485:2016

FREE TRIAL ON MOST INSTRUMENTS

Scan to
Launch Our
Website



103 Estus Drive, Savannah, GA 31404
www.innomed.net info@innomed.net

912.236.0000 Phone
912.236.7766 Fax

Innomed-Europe Tel. +41 41 740 67 74
Fax +41 41 740 67 71

INNOMED

1.800.548.2362