Wixson Hip Positioner

Designed by R.L. Wixson, MD

Provides stable positioning of a patient during hip surgery

The Wixson Hip Positioner is used for stable positioning of a patient during total hip and revision surgery. It is designed to be placed on top of the operating table.

The base plate is rubber-backed to reduce slipping on the table. The uprights can easily be slid in and out of the multiple slots in the plate for desired positioning and locked into position with the locking bolt. The complete upright assembly is radiolucent.

The upright pads and the base plate pad are made of semi-dense foam to help prevent pressure points and are sealed with a washable coating. The coating also helps to lessen the possibility of skin breakdown.

The hip positioner consists of: One 10" post with double pads, one 6" post with a single pad, one 20" base plate, one base plate pad, two 2" spacers, one 4" knob, and one 6" knob.

The spacers and longer knobs are supplied for use with larger patients: use one spacer with the 4" knob, or combine the two spacers to use with the 6" knob.

The pad assembly can be adjusted for additional height and width. The upright posts are modular. The complete unit is radiolucent, and all parts are autoclavable except for the washable foam pads.

Standard Baseplate Dimensions: 20" x 11.25" (50,8 cm x 28,6 cm)

PRODUCT NO'S:	
4050	[Set] *Consists of: One 10" post assembly with double pads, one 6" post assembly with a single pad, one 20" base plate, one base plate pad, two 2" spacers, one 4" knob, and one 6" knob.*
Pads, Pad Parts, Pad Assemblies & Sets:	
4050-LPD	[Large Pad]
4150-CP	[Curved Pad] ***New Option!***
4150-P	[Pad Plate] *(Small Pad Attaches to this Plate)*
4150-PA	[Pad Assembly] *(Pad Knob, Pad Plate & Pad)*
4150-PB	[Pad Knob] *(Attaches Pad Plate to Post)*
4150-PD3	[Set of 3 Small Pads]
4150-PD12	[Case of 12 Small Pads]
4150-V	[Set of 30 Velcro Strips] *(For Pad Attachment)*
Posts, Post Parts, Post Assemblies & Sets:	
4150-06	[6" Post (15,2 cm)] *(Post Only)*
4150-06B	[6" Post with Pad Assembly]
4050-06C	[6" Post with Pad Assembly and Slider]
4150-08	[8" Post (20,3 cm)] *(Post Only)*
4150-09	[9" Post (22,9 cm)] *(Post Only)*
4150-10	[10" Post (25,4 cm)] *(Post Only)*
4150-10B	[10" Post with Pad Assembly]
4050-10C	[10" Post with Pad Assembly and Slider]
4150-12	[12" Post (30,5 cm)] *(Post Only)*
4150-14	[14" Post (35,6 cm)] *(Post Only)*
4050-PA	[Curved Pad Post Assembly] ***New Option!*** *(Curved Pad, Pad, (2) Pad Knobs, (2) Pad Plates, 8" Post)*
4050-PDS	[Full Pad Set] *(1 Large & 3 Small Pads)*
4150-PS	[Post Screw]
4050-S	[Slider] *(Connects Post to Baseplate)*
Extension Parts, Extension Assemblies & Sets:	
4150-C	[2" Spacer (5,1 cm)]
4150-C4	[4" Spacer (10,2 cm)]
4150-EK	[4" Knob (10,2 cm)] *For use with 2" Spacer*
4150-EK4	[6" Extension Long Knob (15,2 cm)] *For use with two 2" Spacers or one 4" Spacer*
4150-EK6	[8" Extension Long Knob (20,3 cm)] *For use with one 2" Spacer and one 4" Spacer*
4150-EXT	[2" Extension] *(2" Spacer with 4" Knob)*
4150-EXT4	[4" Extension] *(4"Spacer with 6" Knob)*
4150-EXT6	[6" Extension] *(4" and 2" Spacers with 8" Knob)*
Baseplates:	
4050-BP	[20" Standard Baseplate (50,8 cm)] *(Baseplate Only)*
4050-BP24	[24" Custom Baseplate (61 cm)] *(Baseplate Only)*

USA MADE

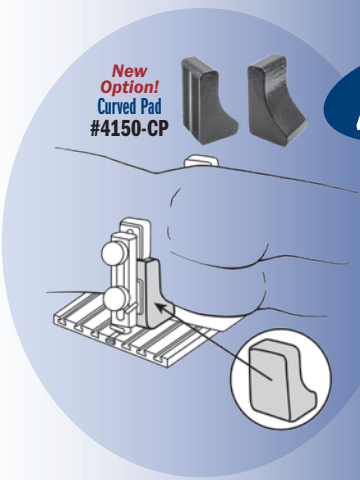

New!

Optional Curved Pad Post Assembly:	
4050-PA	[Curved Pad Post Assembly]
Assembly Includes / Available Separately:	
4150-CP	[Curved Pad]
4150-P	[Pad Plate] *(Pads Attach to this Plate)* ***Two included in set; one only with this product number.***
4150-PB	[Pad Knob] *(Attaches Pad Plate to Post)* ***Two included in set; one only with this product number.***
	[Small Pad]
4150-08	[8" Post (20,3 cm)] *(Post Only)*
Replacement Parts:	
4150-PD3	[Set of 3 Small Pads]
4150-PD12	[Case of 12 Small Pads]

www.innomed.net

FREE TRIAL ON MOST INSTRUMENTS

ISO 13485:2016

© 2026 Innomed, Inc.

103 Estus Drive, Savannah, GA 31404
info@innomed.net

912.236.0000 Phone
912.236.7766 Fax

Innomed-Europe Tel. +41 41 740 67 74
info@innomed-europe.com

1.800.548.2362

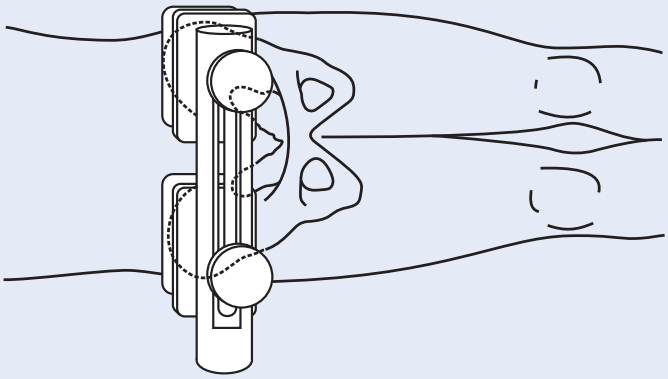

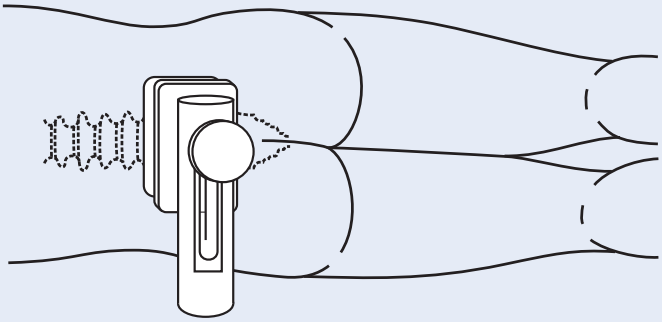

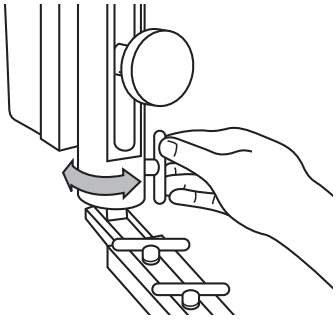

The upright assembly can be rotated and locked in place.

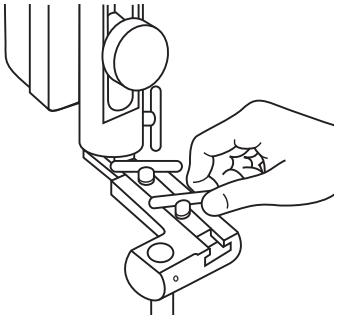

The upright assembly adjusts by a sliding track to accommodate various sized patients. It is locked in the sliding track by tightening one or two locking bolts.

The pads can be adjusted for height and width.

Spacer assembly.

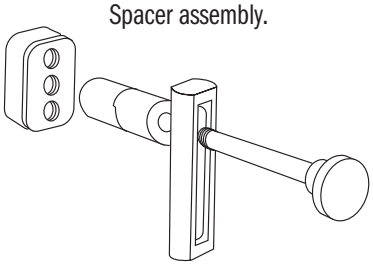
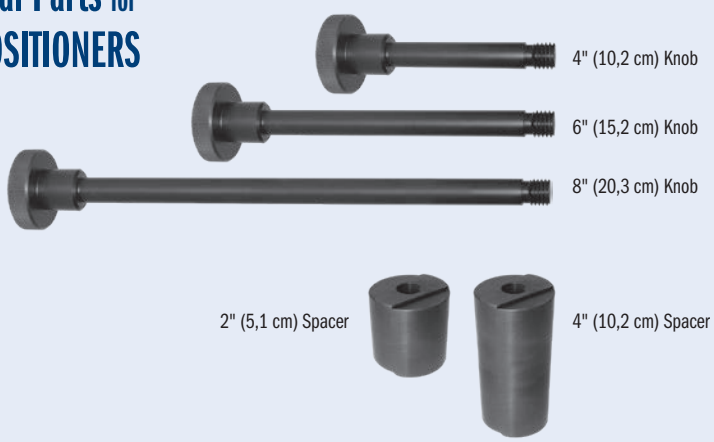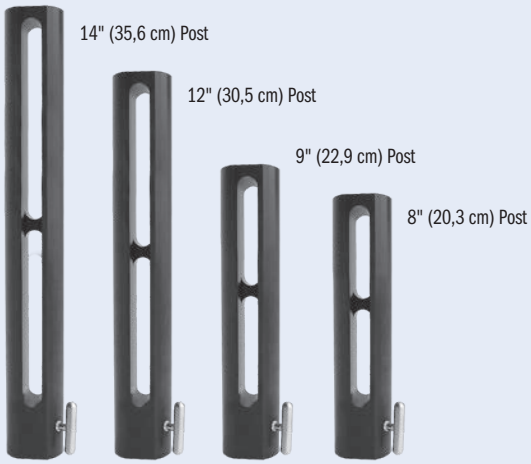
Optional Parts for HIP POSITIONERS